



Agilent Technologies

Sample name: M9651-TLR4-IN-C34-01

Instrument: A010

Inj. volume: 8

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

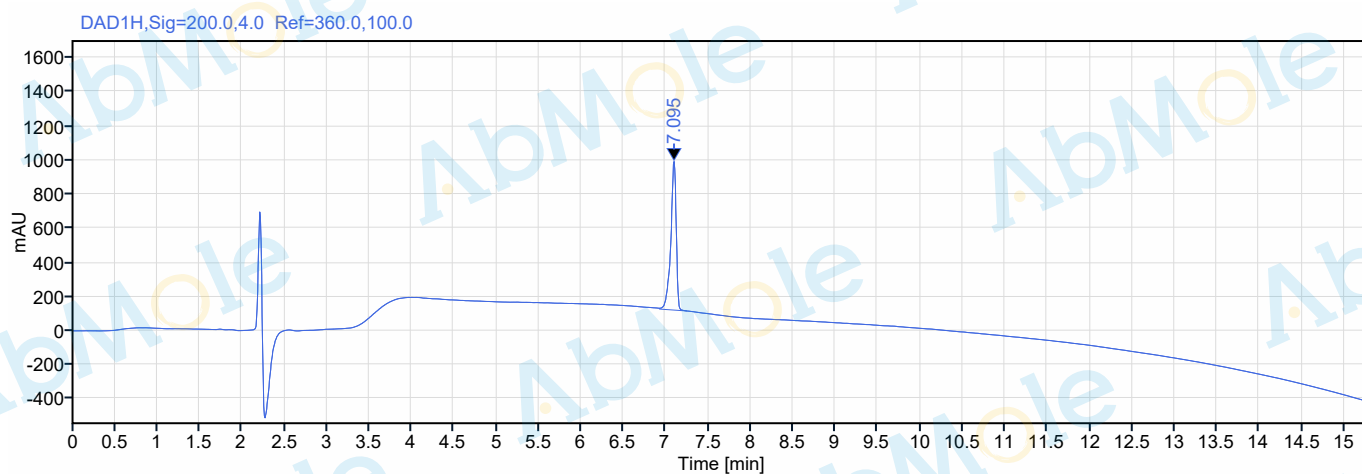

Signal: DAD1H,Sig=200.0,4.0 Ref=360.0,100.0

RT [min]	Type	Width [min]	Area	Height	Area%
7.095	MM m	0.32	3862.17	871.76	100.00