



Agilent Technologies

Sample name: M9727-SBI-115-04

Instrument: A012

Inj. volume: 2

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

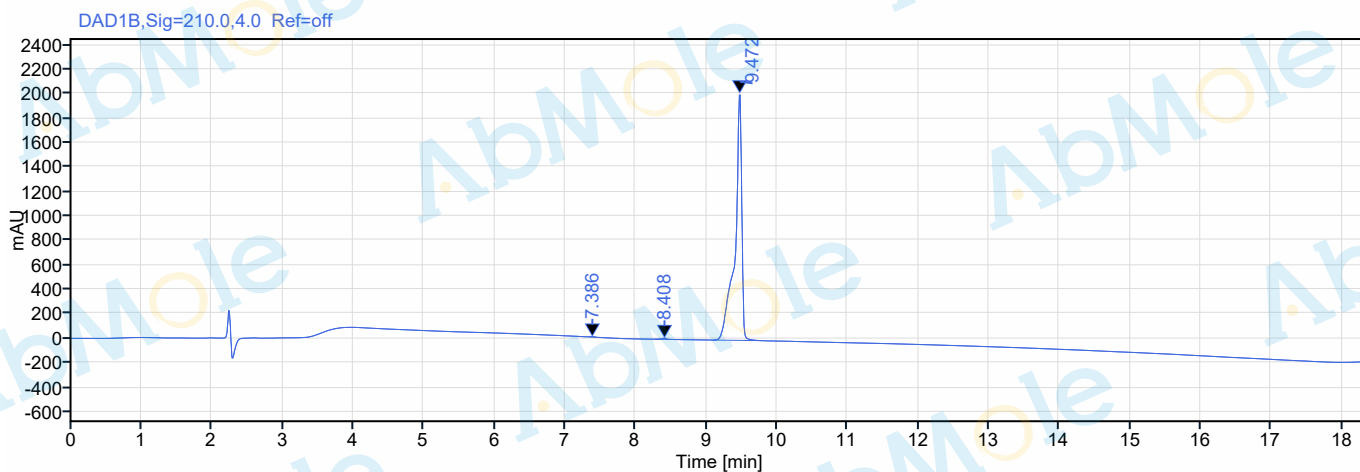

Signal: DAD1B,Sig=210.0,4.0 Ref=off

RT [min]	Area	Height	Area%
7.386	7.92	2.49	0.06
8.408	41.79	9.75	0.31
9.472	13510.37	2018.60	99.63