


```

=====
Acq. Operator   : SYSTEM                      Seq. Line :    6
Acq. Instrument : 0                          Location  : P2-B-06
Sample Name    : M9876-UBCS039-01            Inj       :    1
                                           Inj Volume: 1.000 µl
=====

```

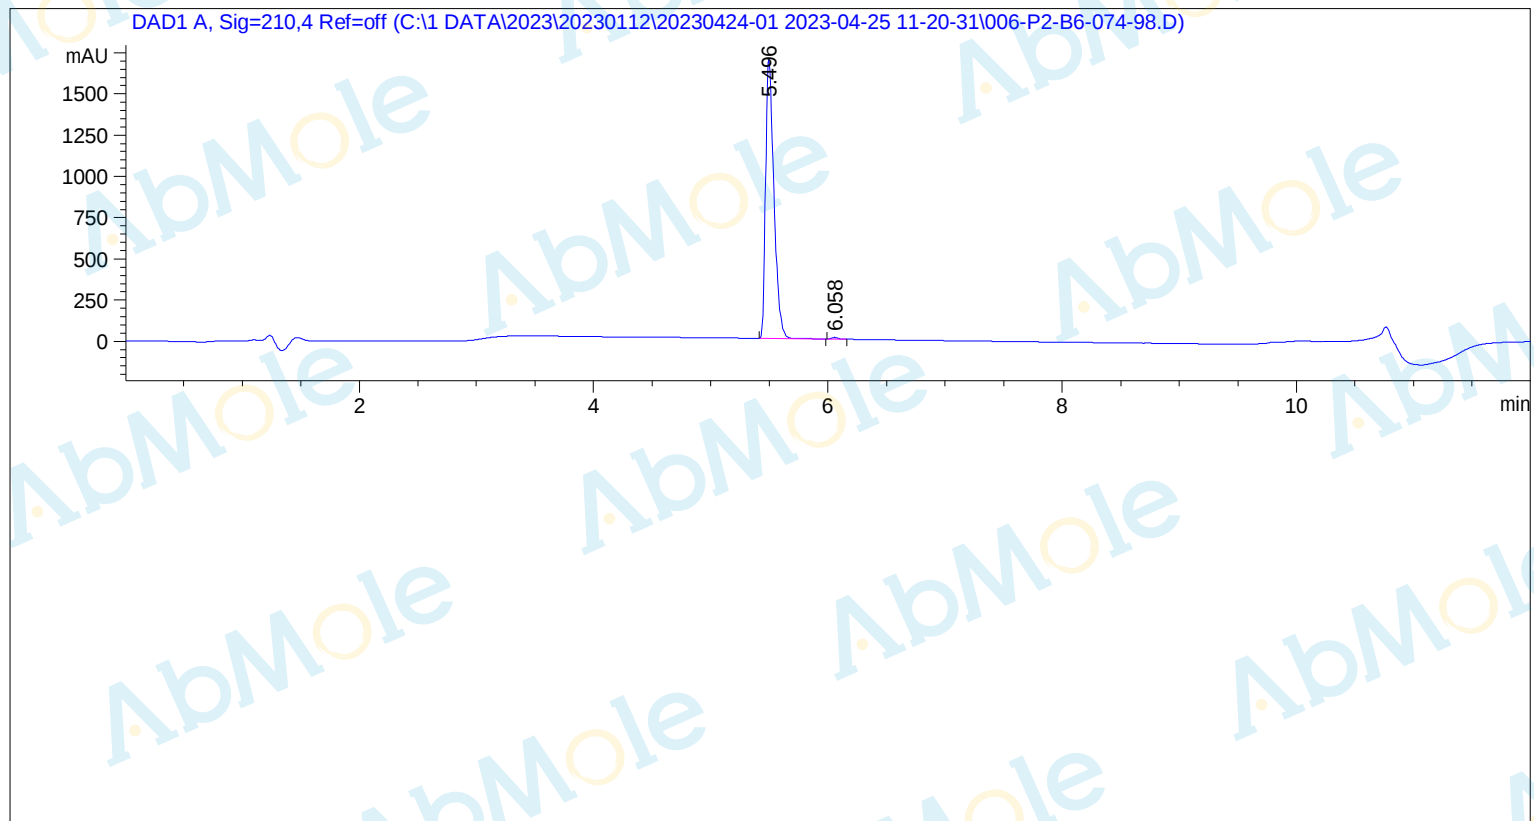

=====
Area Percent Report
=====

```

Sorted By      : Signal
Multiplier     : 1.0000
Dilution      : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

```

Signal 1: DAD1 A, Sig=210,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	5.496	BB	0.0754	8327.43457	1691.38428	99.5543
2	6.058	BB	0.0568	37.28477	10.16832	0.4457

Totals : 8364.71934 1701.55260