



Agilent Technologies

Sample name: M9909-Eltanexor-02

Instrument: A010

Inj. volume: 2

Acq. method: HPLC

Processing method:


Manually modified:

Injection date:

Location:

Type:

Sample amount:

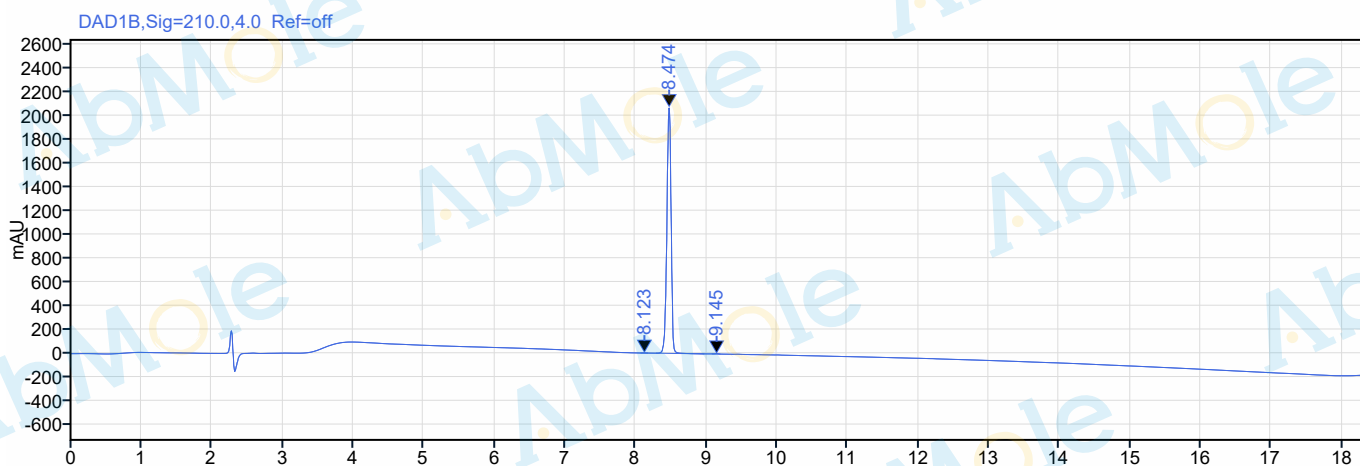

Signal: DAD1B, Sig=210.0, 4.0 Ref=off

RT [min]	Area	Height	Area%
8.123	2.21	0.66	0.03
8.474	8625.41	2075.32	99.88
9.145	7.99	2.36	0.09