


```

Acq. Operator   : System                               Seq. Line :    8
Acq. Instrument : LC1260                               Location  : Vial 28
Injection Date  : 1/19/2017 12:08:56 AM                Inj       :    1
                                                    Inj Volume: 0 µl
Different Inj Volume from Sequence !      Actual Inj Volume : 5 µl
Acq. Method     : E:\DATA\Data\20170117\20160903-01 2017-01-18 21-28-12\0-60 AD 15MIN.M
Last changed    : 1/18/2017 10:49:46 PM by System
Analysis Method : D:\PUBLIC\20170114\DEF_LC 2017-01-14 13-36-10\FCW-0113-02.D\DA.M (10-80 6MIN.
M)
Last changed    : 1/17/2017 10:31:16 PM
                  (modified after loading)

```

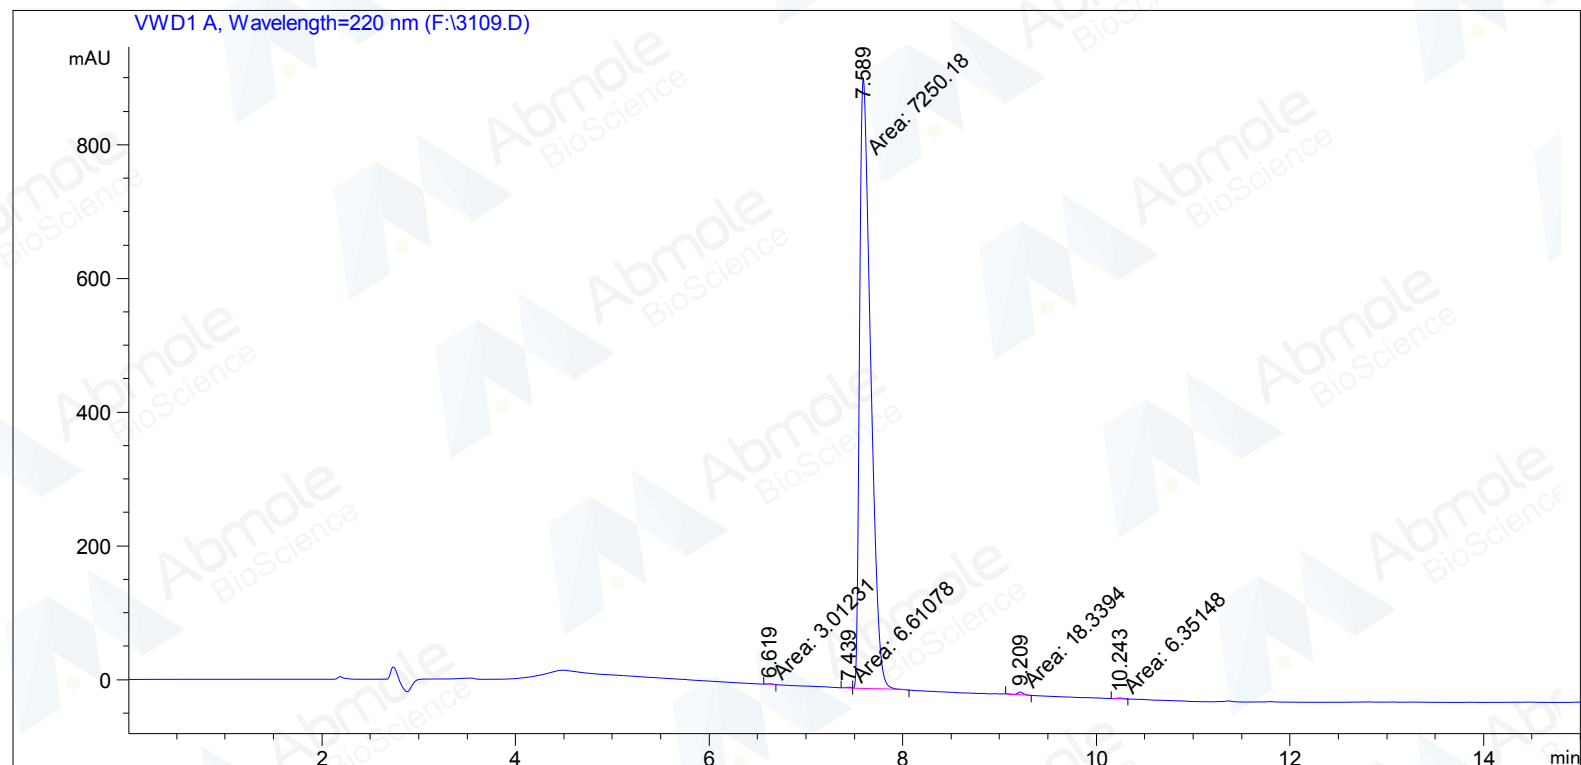

Area Percent Report

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=220 nm

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	6.619	MM	0.0563	3.01231	8.91255e-1	0.0414
2	7.439	MF	0.0737	6.61078	1.49420	0.0908

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
3	7.589	FM	0.1323	7250.18018	913.06952	99.5289
4	9.209	MM	0.0740	18.33942	4.13094	0.2518
5	10.243	MM	0.0807	6.35148	1.31168	0.0872

Totals : 7284.49417 920.89759

*** End of Report ***