


MASS SPECTROMETRY REPORT

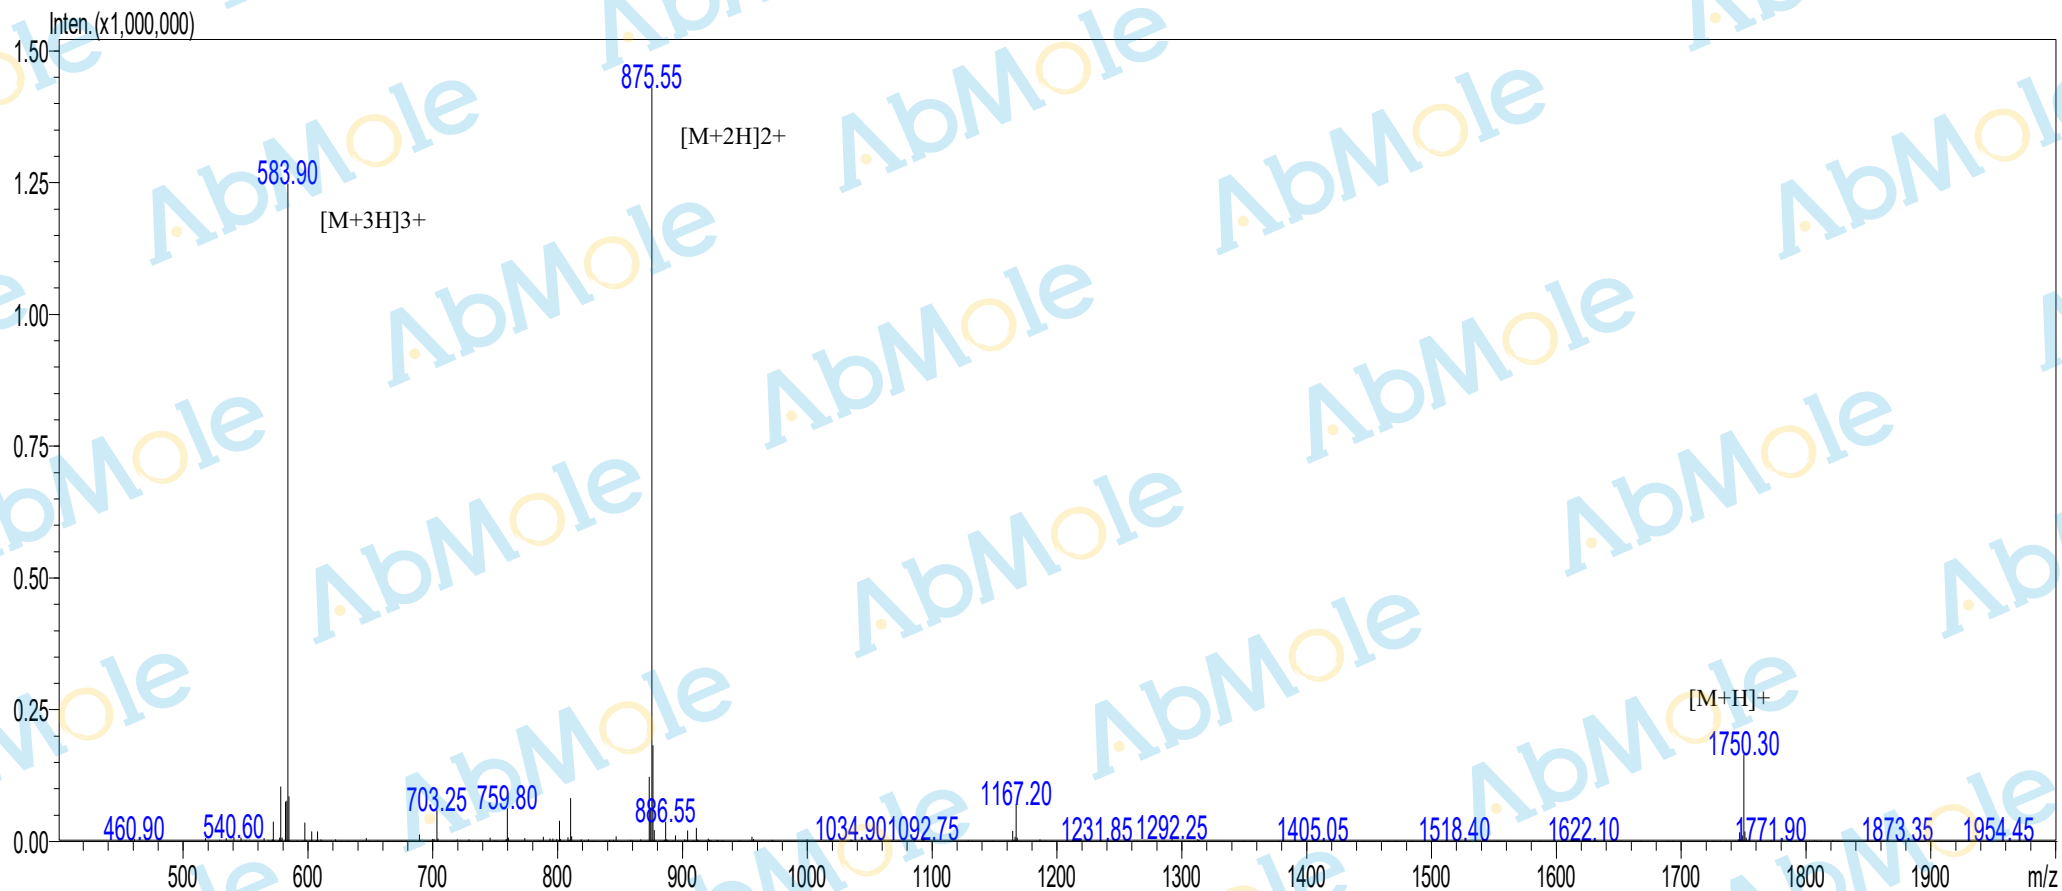

Sample Description

Analyzed date: 2021-1-27
Analyst: SHAO
Sample: OXA (17-33)-01
M.W.: 1749.0
Lot. No.:

Instrument

SHIMADZU LCMS-2020
Probe: ESI
Nebulizer Gas Flow: 1.5L/min
CDL: -20.0v
CDL Temp.: 250°C
Block Temp.: 200°C

SHIMADZU LCMS-2020

Probe Bias: +4.5kv
Detector: 1.5kv
T. Flow: 0.2ml/min
B. Conc.: 50%H2O/50%ACN