

File D:\DATA

Injection Date : 25-May-15, 19:45

Sample Name : MBX-2982-01

Acq. Operator : HPLC

Acq. Method : C:\Chem32\1\METHODS\2-HPLC-15MIN.M

Analysis Method : C:\Chem32\1\METHODS\2-HPLC-15MIN.M

Sample Info :

Method Info : Mobile Phase: A: water(0.01%TFA) B: ACN(0.01%TFA)


Gradient: 0min 5%B,3min 5%B,10min 95%B,15min 95%B

Flow Rate: 1.2 ml/min


Column: Eclipse XDB-C18,4.6*150mm,5um

Oven Temperature: 40 C

DAD1 A, Sig=214,4 Ref=off

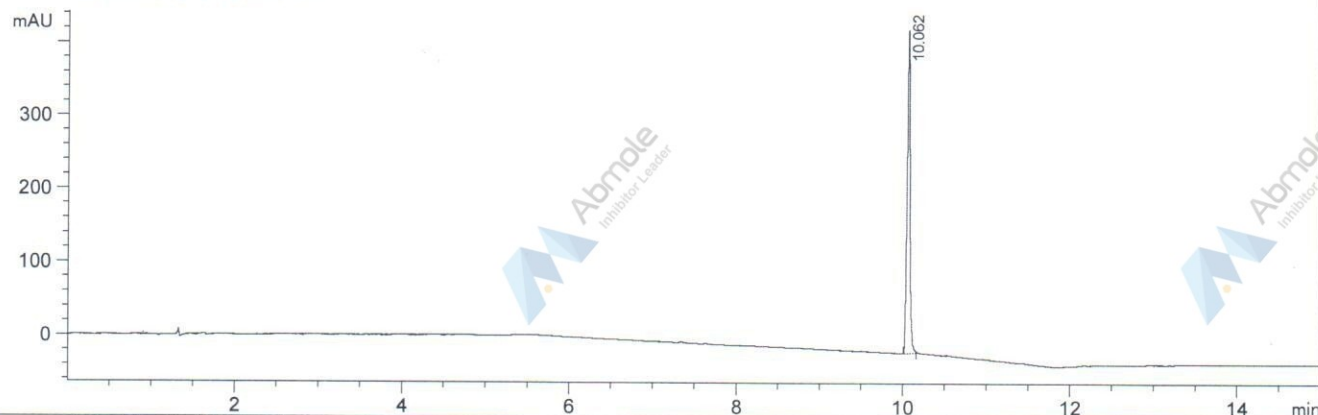

DAD1 B, Sig=254,4 Ref=off

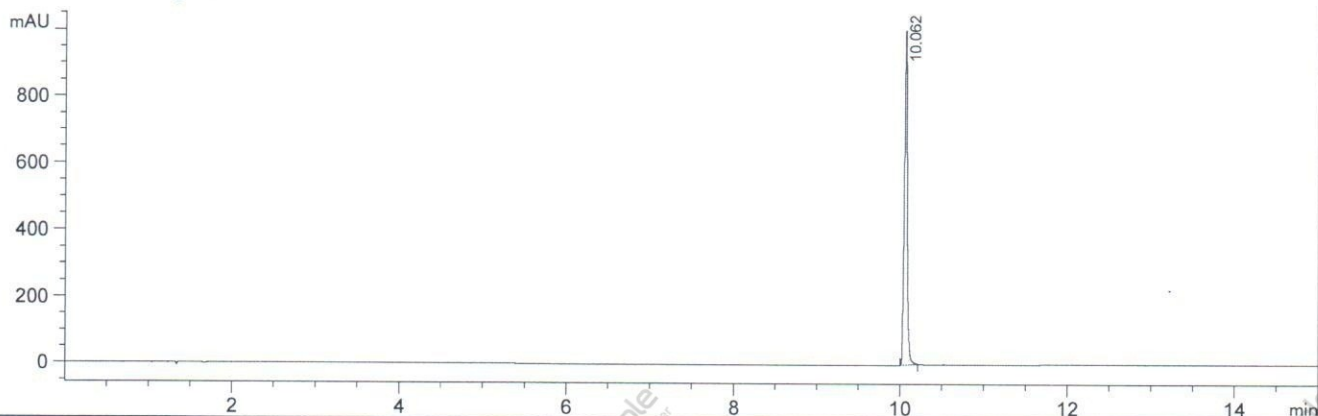

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
10.06	0.04	1055.71	441.16	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
10.06	0.04	2427.18	1001.96	100.00